

田 敬 貴  
縣 齊 德

右 畢 敬 彦

我 以 爲 幸

(2) 臨床検体

福岡県立総合医療センター 福岡市南区 60-8-305



[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]


[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

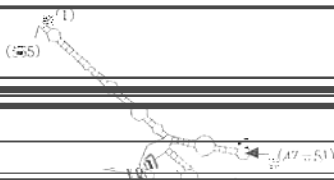

[REDACTED]

[REDACTED]



[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

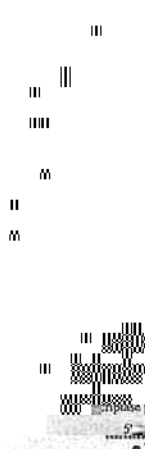

Amplified RNA  
INAR probe  
Fluorescence detection

antigenic  
primer  
5' Target RNA  
Secondary probe  
3'

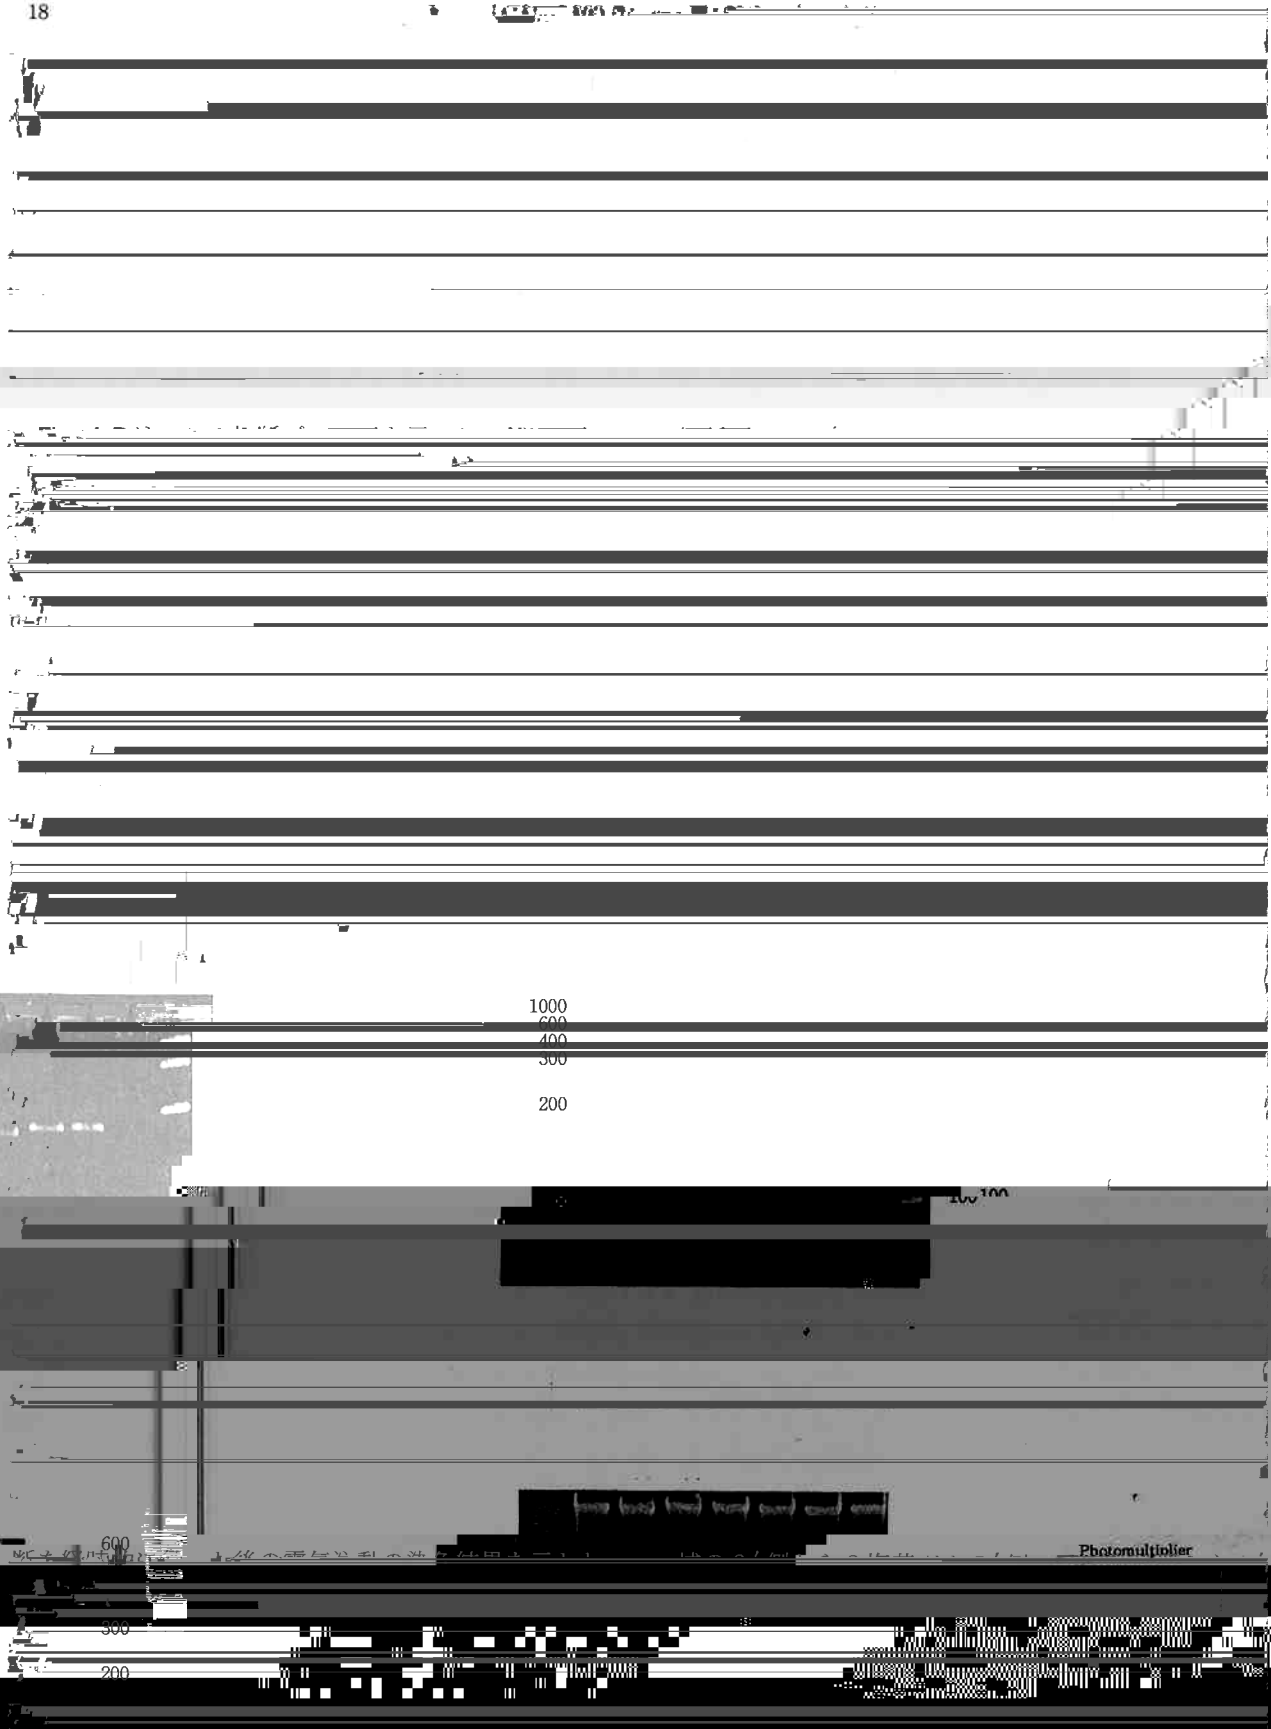


Fig. 4. Analysis of noise spectrum by noise


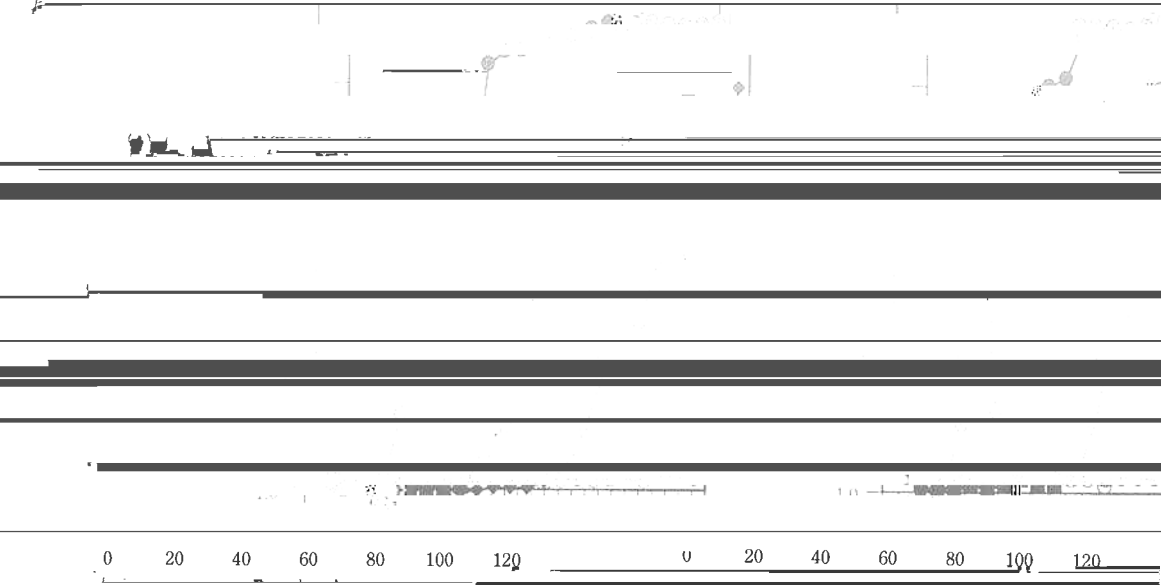


Fig. 6. Real-time monitoring during FPD...

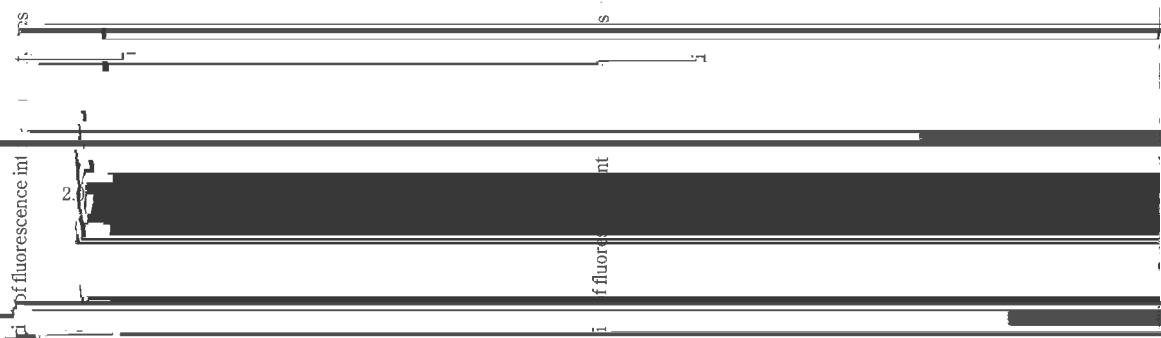

[REDACTED]

[REDACTED]

[REDACTED]

(1996)

-1997. (1996)

[REDACTED]

[REDACTED]

[REDACTED]



[REDACTED]

[REDACTED]